

SERIES: AMT-PGRM | **DESCRIPTION:** PROGRAMMING MODULE**FEATURES**

- for use with AMT Viewpoint™
- USB mini B to USB A cable required
- programming, configuration, and monitoring of compatible AMT encoders
- compatible with AMT11, AMT13, AMT21, AMT22, AMT23, AMT31, and AMT33 Series

**DESCRIPTION**


The AMT-PGRM module is used for programming AMT encoders with the AMT Viewpoint™ software. A programming kit includes the module and one cable. A USB Mini B to USB A cable is also required (not included). Please reference the AMT Viewpoint™ user manual for additional information.

MODEL

	Compatible AMT Encoders	Compatible USB Cables
AMT-PGRM-06C	AMT212, AMT213, AMT222, AMT223, AMT232, AMT233	
AMT-PGRM-14C	AMT113, AMT313	CBL-UA-MB-1, CBLT-UA-MB-1
AMT-PGRM-17C	AMT112, AMT312	
AMT-PGRM-18C	AMT132, AMT133, AMT332, AMT333	


MECHANICAL DRAWING (AMT-PGRM-06C)

units: mm [inch]
tolerance: ± 0.127 mm

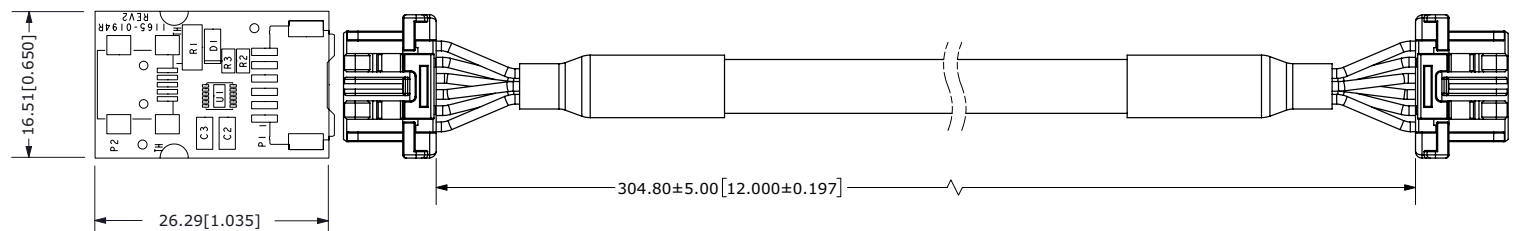


MECHANICAL DRAWING (AMT-PGRM-14C)

units: mm [inch]
tolerance: ± 0.127 mm

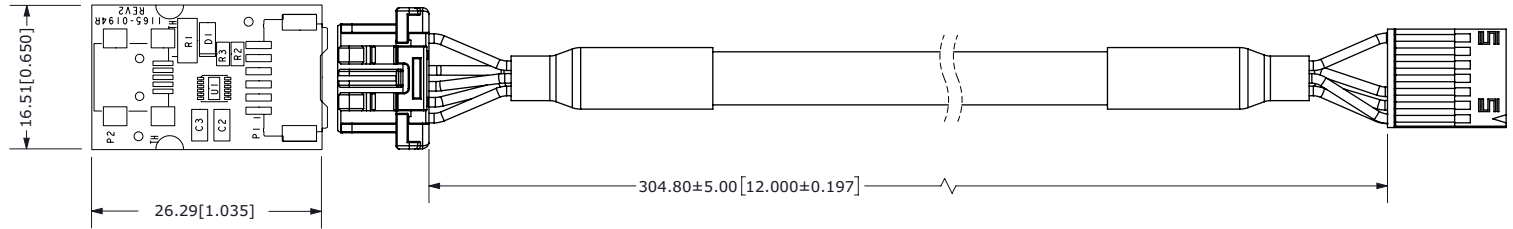


MECHANICAL DRAWING (AMT-PGRM-17C)

units: mm [inch]
tolerance: ± 0.127 mm

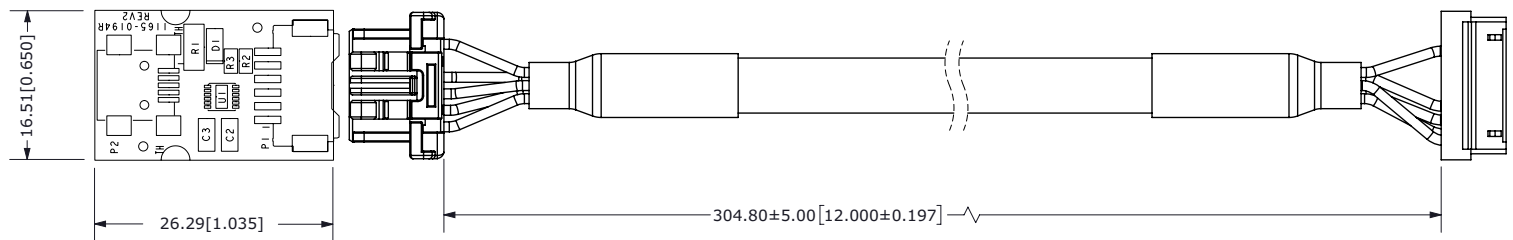

MECHANICAL DRAWING (AMT-PGRM-18C)

units: mm [inch]
tolerance: ± 0.127 mm

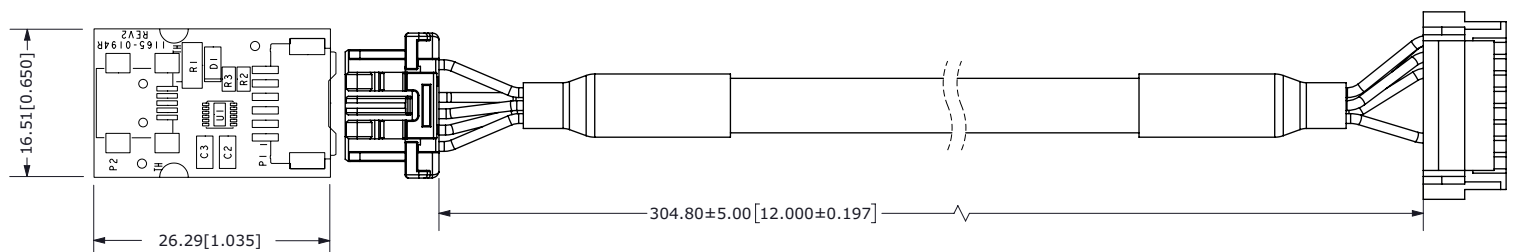

REVISION HISTORY

rev.	description	date
1.0	initial release	07/11/2019
1.01	brand update	02/14/2020

The revision history provided is for informational purposes only and is believed to be accurate.

CUI DEVICES

CUI Devices offers a one (1) year limited warranty. Complete warranty information is listed on our website.

CUI Devices reserves the right to make changes to the product at any time without notice. Information provided by CUI Devices is believed to be accurate and reliable. However, no responsibility is assumed by CUI Devices for its use, nor for any infringements of patents or other rights of third parties which may result from its use.

CUI Devices products are not authorized or warranted for use as critical components in equipment that requires an extremely high level of reliability. A critical component is any component of a life support device or system whose failure to perform can be reasonably expected to cause the failure of the life support device or system, or to affect its safety or effectiveness.